# **SPICER CONSULTING**

ĸĸŧĸĸŧĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸĸŧġŧŧĸŧġŧġĬŧġŧĸŧĸĸĸĸŧſĹġŔġŧţŧĸĸŧĸġŶţĸŧŧĸŧġŧĸŧĸĸſĸŢĘĿĘſĿĸţĸŢŀŔġſĿĸĸĸġŧĸŧġġŔŔĸĿŔĸĸ

# SC11 Sensor Interface Analysis System



- · Windows laptop based measurement and analysis system
- Universal AC power input (100 240 V~)
- Interface with USB connection to laptop, supports multiple sensor types
- Data acquired and pre-processed in Interface
- Inputs for 2 x 3-axis magnetic field sensors, 3 x Wilcoxon 731A accelerometers, Brüel & Kjær precision microphone, analog signals via BNC
- Measures environmental magnetic fields, vibrations and infrasound levels
- Narrow-band and third octave spectrum analysis
- Chart recorder with data logging for long term measurements
- 20 kHz Bandwidth in Scope and Spectrum programs
- Measures 9kHz magnetic fields from wafer transport robots
- Measures DC fields from trams, trains and elevators

# Overview

The SC11/SI is the latest version of our comprehensive site survey equipment. It features data acquisition and preprocessing by an embedded microcomputer in the Sensor Interface for enhanced performance. The separate data acquisition card (DaqCard) used by our earlier systems is not required. The data interface to the computer is through an industry standard USB connection, which enables the system to be used with most modern laptops running Microsoft Windows.

The system is designed to be flexible and adaptable to suit customer requirements. The core system includes the Sensor Interface, Software and a custom carrying case. And a typical system also includes a DC-13 kHz three axis magnetic field sensor, an accelerometer and a precision microphone.

The software suite includes three virtual instruments, an oscilloscope, a spectrum analyser and a chart recorder that display results graphically on the laptop screen. Also included are "SCplot", a comprehensive results plotting program, "SC11 Wizard", which aids in setting up a single measurement, and "SC11 Survey", which automates a complete survey.

# SC11/SI Hardware

## Laptop computer

Typically, our customers use their own laptop computer, purchased in their own country to ensure the correct language and type of keyboard and they install the SC11 software themselves. However, if required, Spicer Consulting (or one of our trained agents) can install the system on the customer's computer or supply a suitable laptop with the system.

The requirement for the computer is Windows XP/Vista/7/8/8.1/10, screen pixels at least 1024 x 768, USB and CD/DVD drive. The processor, RAM and hard drive must be as recommended for the operating system.



Brüel & Kjær 4190 microphone

Wilcoxon 731A accelerometers (up to three)

## Sensor Interface

The Sensor Interface operates from universal AC power (100-240 V  $\sim$  50/60 Hz) which is used to power all the sensors and its embedded Analog Devices Blackfin microcomputer. For long term monitoring applications, where loss of data would not be acceptable, the sensor interface can be powered from an un-interruptible power supply. Our tests with a fully charged 350W UPS from APT provided up to four hours of operation.

There are inputs for two Spicer Consulting 3-axis magnetic field sensors. Sensor SC24/DC+AC and Sensor SC11/AC are compatible. If two sensors are used we recommend they are the same type to avoid confusion.

There are inputs for three Wilcoxon 731A accelerometers. The inputs provide the constant current load and power supply for each Wilcoxon 731A and are suitable for most other types of piezo accelerometers when using the spectrum program.

There is an input for a Brüel & Kjær 4190/2669L precision microphone. The Interface provides the special power supplies for the 2669L microphone pre-amplifier to enable the microphone to operate to its full specification.

There is a general purpose DC coupled auxiliary input via a BNC connector at the back of the interface.

A multi-channel 13 bit ADC controlled by an embedded Analog Devices Blackfin Microcomputer acquires all the signals in digital format inside the Interface. The microcomputer performs extensive signal pre-processing before the signals are sent to the laptop computer through the USB connection.

## Sensor SC24/DC+AC

This is the 3-axis magnetic field sensor most commonly used with the SC11/SI/USB system. It can measure DC and AC fields, e.g. changing DC fields from trams and elevators and AC power line fields. It has internal bias coils that are used to null the Earth's field. The bias coil currents are reset by clicking an icon on the program screen, each time the sensor is moved. The measurement range is  $\pm 20$  mG. The sensor has low noise and when fully warmed up the DC drift is below  $20\mu$ G/day. It is not recommended for measuring higher frequency fields (e.g. 9kHz from wafer transport robots). Sensor SC11/AC should be used for this purpose. (The MEDA uMAG-01N one-axis DC magnetometer is also supported).

#### Sensor SC11/AC

This is a 3-axis AC magnetic field sensor with a lower bandwidth of 1 Hz and a dynamic range of 80 mG (8 mT) Pk-Pk.

#### Wilcoxon Research model 731A accelerometer

The Wilcoxon Research model 731A has a measurement range of 200 mg's Pk-Pk and a bandwidth of 0.1 Hz to 500 Hz when used with SC11/SI/USB system. It is suitable for the measurement of extremely low level vibrations. Its noise limit is  $0.03\mu g/\sqrt{Hz}$  at 2Hz. The system supports simultaneous measurements by three accelerometers. Each accelerometer measures along one independent axis. With three correctly oriented accelerometers, vibration can be measured in three orthogonal axes.

#### Brüel & Kjær 4190/2669L microphone

The Brüel & Kjær 4190 microphone with 2669L preamplifier connects directly to the sensor interface. It provides acoustic measurements to acoustic laboratory reference standards. It measures sound levels from 20dB to 110dB and 1.5Hz to 20kHz. It measures infrasound levels (i.e. frequencies below 20Hz) which can limit the performance of transmission electron microscopes by vibrating the sample. (The Sound Level Meter supplied with the SC11/Compact is also supported).

## Calibration

The magnetic field sensors are manufactured and calibrated by Spicer Consulting. Their calibration is NAMAS traceable.

The Wilcoxon accelerometers are supplied by Wilcoxon Research Inc. Germantown MD, USA with a calibration certificate traceable to the National Institute of Standards and Technology, Gaithersburg, MD, USA.

The Brüel & Kjær 4190 microphone is supplied with a calibration certificate traceable to the National Institute of Standards and Technology, Gaithersburg, MD, USA.

Spicer Consulting provides a re-calibration service for the entire system.

## SC11 5.6 Software

The three SC11 programs, oscilloscope, spectrum analyser and chart recorder run one at a time. (If you try to run more than one, the software will generate an error message telling you the system is already in use.)


The SC11/SI/USB hardware supports operation in 4 channel or 8 channel modes. In 4 channel mode the channels are called X, Y, Z & A. In 8 channel mode the channels are called X1, Y1, Z1, A1, X2, Y2, Z2 & A2. The sensors are assigned to the channels in the calibration window. Many combinations are possible. It is not necessary to have sensors assigned to all the channels in either 4 or 8 channel modes. So for example, you can run in 8 channel mode without a second magnetic field sensor plugged into channel 2.

The principal use for 8 channel mode is to measure real time AC and DC magnetic field gradients by using two magnetic field sensors. This is a unique capability of this system. There are some differences in performance between the 4 and 8 channel modes. In 8 channel mode the system is acquiring twice as much data and this causes some bandwidth reduction in the chart recorder, a restriction on the choice of points in the spectrum analyser and poorer anti-aliasing performance.

Sensor Interface	Serial Number 09998	
Jensor Interface		
3-axis Magnetic	Sensor 1: SC20/DC S/N 08997 🕞	
	Sensor 2: SC20/DC S/N 03122 🗨 Reset DC Se	nsor
Vibration 1	Wilcoxon 731A SN: 1054	
	Wilcoxon 731A SN: 1067	
Vibration 3	Wilcoxon 731A SN: 1544	
Acoustic	B&K Microphone 4190-L-001 S/N	k
1-axis Magnetic	MEDA uMAG-01N S/N 5155 💽 Range (mG) 20	•
	Add Sensors	

## Oscilloscope

The oscilloscope program is useful for initial investigation of magnetic fields during trouble shooting of electron microscope imaging problems. Examples of oscilloscope screen displays in 8 channel mode are shown below.

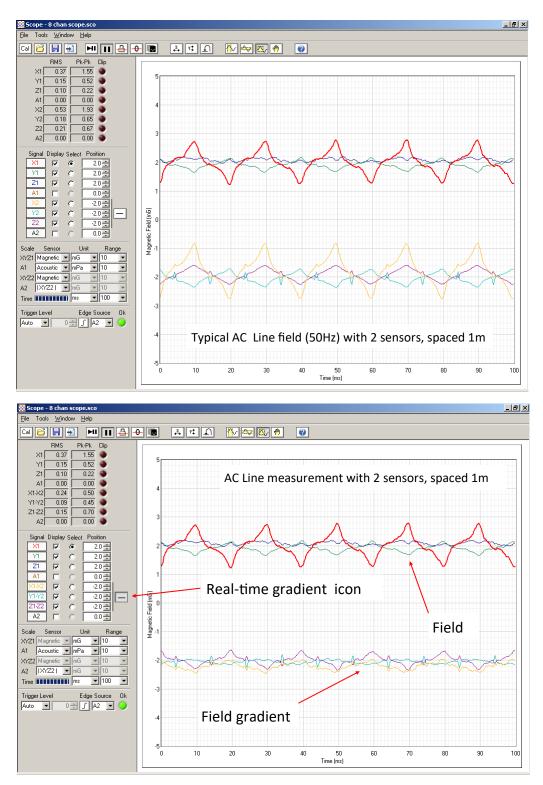


The oscilloscope has a bandwidth of 20kHz on its shorter time ranges. The A input is DC coupled. There are common controls for the time base and the vertical axis ranges. There are independent controls for the auxiliary channel ranges and the vertical position of each channel. The RMS and Pk-Pk values of the waveforms are measured and displayed numerically.

Icons on the top toolbar are used to control operation. These include "pause", "one-shot", "reset DC sensors" and "zero position". The "lock position" icon activates AC coupling that varies with the time base. The effect is to stabilise the vertical position of the traces, which is useful with an AC sensor that is being moved frequently during searches for magnetic field sources.

Files to set-up the controls may be imported and exported for future use. Results may be saved as an image using the windows alt-print-screen function or exported as a text file or Matlab level 5 file for processing by the SCplot program.


## Spectrum Analyser

The spectrum analyser program enables in-depth analysis of magnetic field, vibration, sound and other sources such as the video output from an SEM in spot-mode. It displays the waveforms and spectra of up to 8 channels. It highlights the selected channel. It has a wide range of units for use with all the sensors. An example of floor vibration analysis using 3 Wilcoxon 731A accelerometers is shown below. When measuring vibration with the Wilcoxon 731A accelerometer, the software integrates its output to provide velocity and displacement units as well as acceleration.

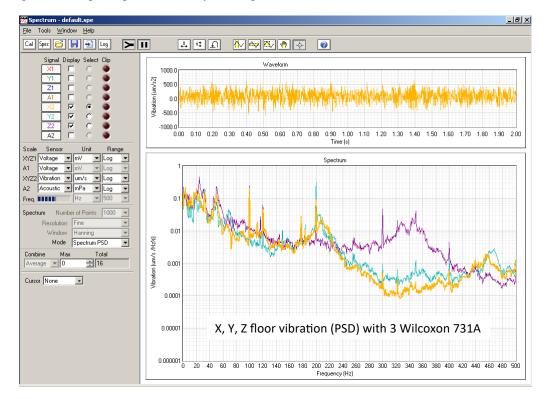

Tracking cursors are provided to measure features of the spectrum as well as define bands for RMS measurement. Harmonic cursors can be used to recognise harmonics in the spectrum and enable more accurate measurement of the fundamental frequency. Successive spectra can be combined over a period of time, as an average to reduce noise, or to find the worst case peak values. Spectra can be data-logged to a file at a maximum rate of once every minute to trace sources that vary.


The example below is a sound level measurement with comparison to the Electron Microscope manufacturer's specification, in third octave format. The specification line changes colour from grey to magenta if the specification is exceeded, as shown.

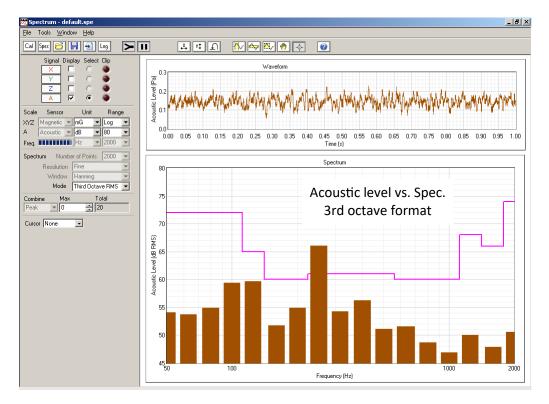


## **Chart Recorder**

The chart program is used to record events that change relatively slowly. It simulates plotting on a paper chart which is up to 20 screen pages wide. It displays in page mode (one screen width at a time) or as a continuous scroll. The most recent 20 pages of data are retained in memory (2 hours 46 minutes at slowest chart speed). Controls for vertical range, chart speed and bandwidth are provided. Pan and zoom controls enable any section of the plot to be examined. You can mark events that occur during measurement of any chart, such as the movement of trains. The markers are exported with the results.

The example below, in 4 channel mode, is a chart of the total Pk-Pk AC magnetic field in the 1Hz to 2500Hz range. The program is calculating the Pk-Pk values in real time and charting the result. It shows that the X field was steady at 1.05mG Pk-Pk and the Z field varied from 0.1 to 0.3mG Pk-Pk during the 100 second period of the chart. By selecting the narrow band option the program can chart the field at a specified frequency, e.g. 50Hz or 60Hz.

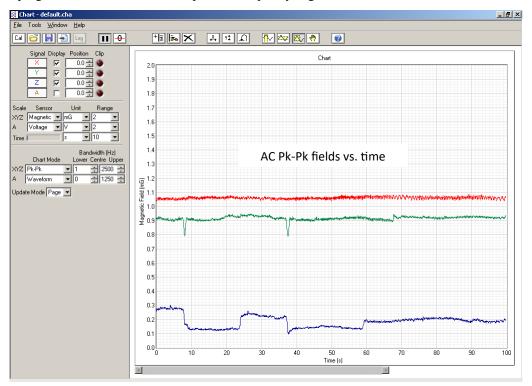


The waveform chart below was recorded in 8 channel mode using two SC24/DC+AC sensors and DC-1250Hz bandwidth. The "width" of each trace is the Pk-Pk value of the AC power line fields (50Hz and harmonics), so the X1 axis power line field is 0.8mG Pk-Pk. The step function changes are the DC field caused by to the movement of nearby steel objects, in this case, about 4 mG Pk-Pk in X1. This "combined" charting mode was a new feature in the SC11 software version 5.0.

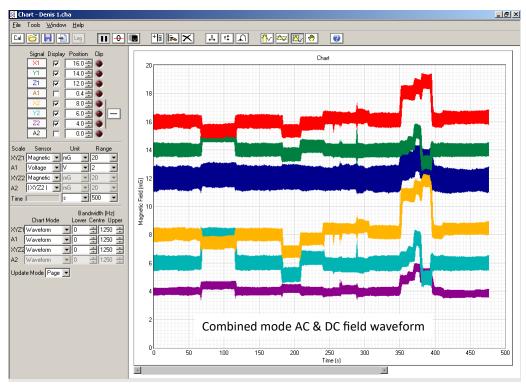

6

The results of two consecutive acoustic measurements (without moving the microphone) are shown below. First is in the audible range (40-2500 Hz) second in the infra sound range (1.5-40 Hz). Note that the infra-sound level is typically higher. Infra sound can seriously degrade the performance of high end TEMs by moving the sample. The Brüel & Kjær 4190 microphone enables accurate infrasound measurements to below 2 Hz.

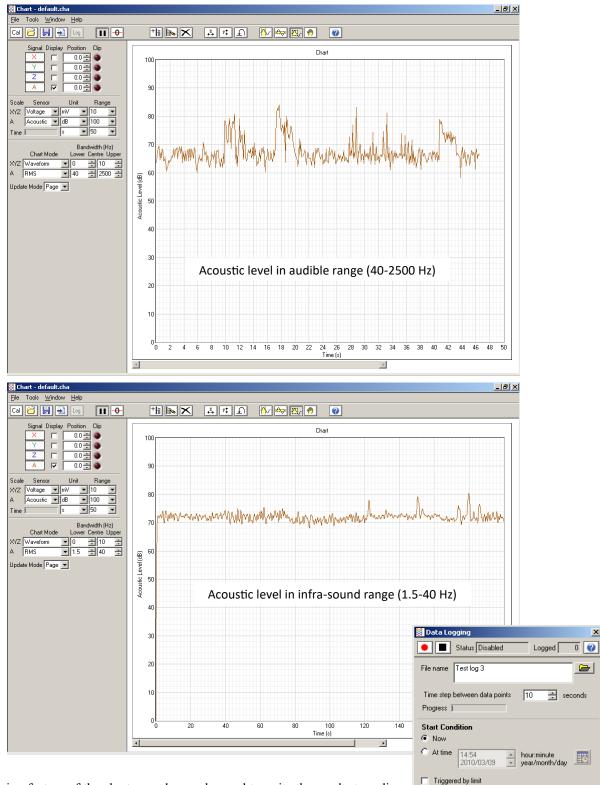


The data logging feature of the chart recorder can be used to write the results to a disc file at a specified rate, as the data is acquired. This is useful for long term recording of disturbances that occur occasionally or overnight. The adjacent screen image shows the comprehensive start and stop controls for data logging.



x

When charting vibration using the 731A accelerometers, an integrating filter tailored to the 731A allows direct displacement and velocity charts to be made. This is useful for "walk about" floor vibration tests at proposed electron microscope sites, as in the example below.

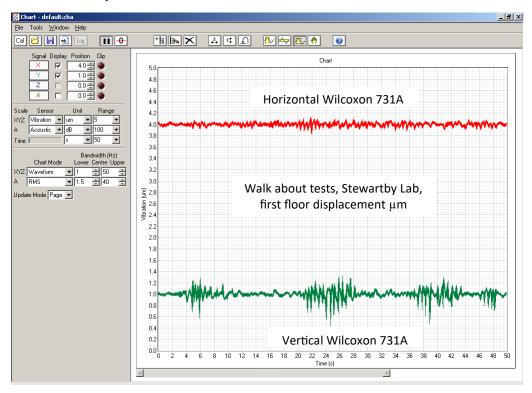


## **SCplot**

SCplot is a comprehensive results editing program that enables results exported as text files or Matlab level 5 files from the Oscilloscope, Spectrum and Chart recorder programs to be formatted for published reports. It is particularly useful for formatting the large text files that result from long term data logging.

It supports all the units and formats that are used in the Oscilloscope, Spectrum and Chart recorder programs. It enables units conversion and can post-process results with user specified formulas. SCplot can show multiple results measured at different times on a 3D waterfall plot and it can append plots to a document in Microsoft Word.

The acoustic measurement shown on page 5 is reproduced below as an image exported from SCplot after formatting.

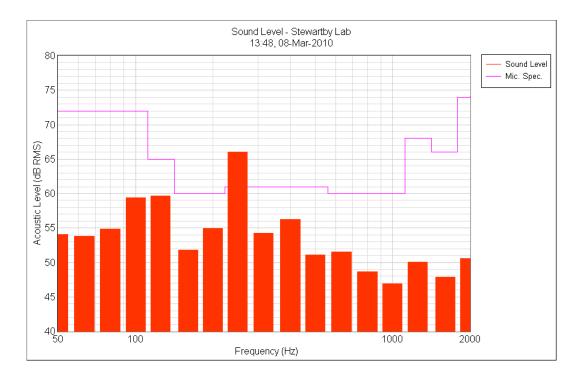

## SC11 Wizard

The SC11 Wizard quickly and easily starts predefined measurements using one of the three measurement programs. It guides you through the choice of sensors, the instrument for which the environment is to be checked, the type of analysis and the type of measurement.

The Wizard helps new or occasional users to get started with making measurements as simply as possible, using setup files that have already been created by an expert user. It also helps experienced users to organise their setup files.


## SC11 Survey

SC11 Survey automates a complete survey by calling the SC11 instruments using Active X technology. It is like the SC11 Wizard except that it uses a macro that can run several measurements and automatically save the results. Survey guides you through the choice of sensors, a self test to ensure all the sensors are working and then the survey itself. Survey enables first-time users to set up the equipment and run a standard survey using a macro and setup files that have already been created by an expert user.

This program is designed to work with the full SC11/SI system with 2 DC magnetic field sensors, 3 accelerometers and a precision microphone. Self test can be customised to omit magnetic field, or vibration or acoustic tests if required. Survey macros are very flexible, but once written, they require the sensors for which they are designed.

The Show Presentation button on the Start page opens a document that shows in detail how to connect the sensors, run a self test and perform a survey for the full SC11/SI system. It is possible to customise this presentation for other hardware configurations.

Self test works by comparing the output of 2 magnetic field sensors or 3 accelerometers. It also uses the self-test feature of the precision microphone. The self test report includes

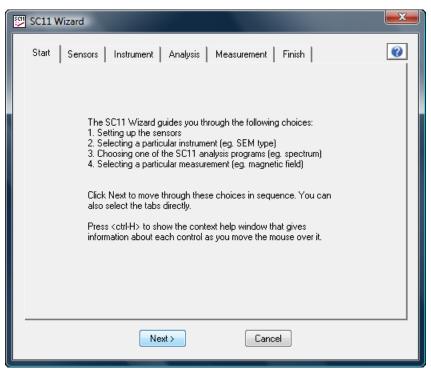

SC11 Survey	×
Start Sensors SelfTest Survey Finish	<b>@</b>
SC11 Survey guides you through the following choices: 1. Setting up the hardware sensors 2. Selecting the sensors in the software 3. Running a self-test to confirm the sensors are working 4. Running a survey	
Click Next to move through these choices in sequence. You can also select the tabs directly. Press <ctrl-h> to show the context help window that gives information about each control as you move the mouse over it.</ctrl-h>	
Show Presentation Guides you through the whole process.	
Next > Cancel	

spectra comparing the sensors and a pass/fail result. If self test fails, it advises the user to ask for support before continuing with the survey. The report can then be sent to an expert user so that they can diagnose whether a sensor is faulty or advise the user how to get it working.

To run a survey, the user follows the instructions in the presentation and then selects the required survey from a predefined list. Surveys may be repeated at fixed intervals to show how the environment changes with time. SCplot can show this in a waterfall plot.

Survey macros are written by an expert user as follows: First set up a measurement in the scope program and save the setup file. Then turn on macro recording and run through the process of loading the setup, making the measurement and saving the results. Save the macro. Repeat for the spectrum analyser and chart recorder. Do the same with SCplot to create the graphs required and append them to a survey report in Microsoft Word. Manually edit the recorded macros together, adding Wait and Exit statements to make a complete survey macro. Save the setup files and the macro together in a folder ready for SC11 Survey to use. Macros contain simple statements that run in sequence. However the statements can be directly used in Microsoft Visual Basic if more complicated programming is required.

# **SC11/SI - Specification**

#### System

Carrying Case Size

Weight

58 x 36 x 19 cm approx. (23 x 14 x 7.5 in approx.) 11 kg (24 lb) approx. including typical laptop.

At least 1024 x 768 pixels

As required for operating system

As required for operating system

As required for operating system

USB 1.0 or 2.0

CD/DVD

#### Laptop Personal Computer Windows XP/Vista/7/8/8.1/10

Operating System Display Interface Optical Drive Processor Memory Hard Disc

#### Core System: SC11/SI (Sensor Interface)

Inputs

Power

MAG1, MAG2 VIB1, VIB2, VIB3 MIC AUX

3-axis vibration (3 x Wilcoxon 731A) Microphone (B&K 4190/2669L) BNC voltage input, DC coupled, ±10 V range 100 k $\Omega$  impedance. 20kHz 100-240V AC, 50-60 Hz, 0.25A max

3-axis magnetic field sensor (2 x SC sensor)

#### 3-axis Magnetic Field Sensor: SC24/DC+AC

Co-ordinate System Bandwidth Ambient Field Range Measurement Range Warm-up drift

Long term drift

Noise Level

Accuracy

Anti-aliasing Filters

X, Y, Z rectangular Cartesian DC - 13kHz ±2000 mG (±200 µT)  $\pm 20 \text{ mG} (\pm 2.0 \mu \text{T})$  $\pm 0.1$ mG ( $\pm 10$  nT ) in 2 hours (typ)  $\pm 0.25$  mG ( $\pm 50$  nT ) in 2 hours (max)  $\pm 20 \ \mu G \ (\pm 2 \ nT)$  in 24 hours 7  $\mu G \ (0.7 nT)$  RMS (0 - 10 kHz)  $\pm 1$  % (after >2 hour warm up). ( $\pm 5$  % cold)

3-axis Magnetic Field Sensor: SC11/AC

Co-ordinate System Bandwidth Measurement Range Noise Level Accuracy

X, Y, Z rectangular Cartesian 1 - 20 kHz 80 mG (8 µT) Pk-Pk 3µG (0.3 nT) RMS max

#### Vibration Sensor: Wilcoxon 731A Accelerometer

Туре Bandwidth Measurement Range Noise Limit

Accuracy

Help

Wilcoxon Research, model 731A 0.1 - 500 Hz 2 m/s<sup>2</sup> (0.2 g's<sup> $\alpha$ </sup>) Pk-Pk (in this system) 7 µm/s<sup>2</sup> RMS max. 0.35 µm/s RMS at 1Hz, 0.11 µm/s RMS at 5Hz  $0.07~\mu m$  RMS at 1Hz,  $0.0035~\mu m$  RMS at 5Hz  $\pm 5$  % (with gain calibration file)

#### Acoustic Sensor: B&K 4190/2669L Microphone Brüel & Kjær, Condenser microphone 4190,

Type Bandwidth Measurement Range Noise Limit Accuracy

#### **Programs (General)**

Channel modes 4 channel & 8 channel 4 channel mode X, Y, Z, A 8 channel mode X1, Y1, Z1, A1, X2, Y2, Z2, A2 Audio/visual indication Channels Clipping Pause control Freeze/resume instrument operation Calibration panel Set channel mode, add/select sensors, set ranges, calibrate offsets, microphone self check, add/edit user defined units, set export file options. Setup file Open/save instrument controls Export results for SCplot or spreadsheet Export Print window Print current screen display Context help on controls, online help file

Pre-amplifier 2669L 1.5 Hz - 20 kHz 110 dB (in this system)

20 dB (in this system)

±1 dB 3 Hz - 20 kHz

#### Oscilloscope Amplitude units

Magnetic Field Vibration Acoustic Voltage Resultant |XYZ| Time ranges (ms)

Bandwidth (Hz)

Digital Meter Trigger Capture indicator

#### Spectrum Analyser

Displays Select Amplitude units Magnetic field Vibration Acoustic Voltage Resultant |XYZ| Amplitude ranges Frequency ranges

### Number of points

Accuracy Waveform windows Spectrum modes

Combine spectra Cursor modes

Capture indicator Specification files

Data logging

## **Chart Recorder**

Position Amplitude units Magnetic Field Vibration Acoustic Voltage Resultant |XYZ| Page length Chart length Max Bandwidth Magnetic field

Vibration Acoustic (B&K mic.) Voltage Bandwidth controls Narrow band filter

Chart modes

Markers Clear Buffer indicator Update modes Chart palette Data logging

mG, nT, µT, mA/m, A/m  $\mu g's^{\alpha}$ , mg's<sup> $\alpha$ </sup>,  $\mu m/s^{2}$ , mm/s<sup>2</sup> mPa, Pa mV, V, user defined units Magnetic Field, Vibration, Voltage units 0.5, 1, 2, 5, 10, 20, 50, 100, 200, 500, 1000, 2000, 5000 20,000 for time ranges 0.5, 1, 2, 5 At least 100,000/(time range) for other time ranges RMS, Peak to Peak (all channels)

Auto/Manual level, +/- edge, source, one-shot Indicates progress of data acquisition

Waveform (autoscaling), Spectrum Highlight and attach cursor to selected signal

mG, nT, uT, mA/m, A/m  $\mu g's^{\alpha}$ ,  $mg's^{\alpha}$ ,  $\mu m/s^{2}$ ,  $mm/s^{2}$ ,  $\mu m/s$ , mm/s, nm,  $\mu m$ mPa, Pa, dB, dBA, dBC mV, V, user defined units 

 Ivragnetic Field

 1, 2, 5, 10, 20, 50, 100, 200, 500, log full scale.

 20, 25, 30, 40, 50, 60, 80, 100, 120, 160, 200, 250,

 300, 400, 500, 600, 800, 1000, 1200, 1600, 2000,

 2500, 3000, 4000, 5000, 6000, 8000, 10000,

 12000, 16000<sup>β</sup>, 20000, Hz full scale.

 200, 250<sup>°</sup>, 4000, 500<sup>°</sup>, 800, 1000<sup>°</sup>, 1600, 2000<sup>°</sup>,

 3200<sup>β</sup>, 4000<sup>β</sup>

 Frequency ± 0, 010<sup>°</sup> ± 0, 020<sup>°</sup>.

Magnetic Field Frequency: ±0.01% ±0.02 div None, Hanning, Flat top RMS, 0-Pk, Pk-Pk, PSD, Third Octave (RMS, 0-Pk, Pk-Pk) Average/Peak, Max no. spectra Total RMS between 2 tracking cursors, 10 harmonic cursors Indicates progress of data acquisition Create, edit, add & remove. Compare with measurements. Start: Now, At time, Triggered by flat level, Triggered by spec

Stop: Period, File size, Disk space Min. time step: 1 minute

Set or zero vertical positions

mG, nT, µT, mA/m, A/m  $\mu g's^{\alpha}, mg's^{\alpha}, \mu m/s^2, mm/s^2, \mu m/s, mm/s, nm, \mu m$  mPa, Pa, dB, dBA, dBC mV, V, user defined units Magnetic Field, Vibration, Voltage units 5, 10, 25, 50, 100, 250, 500 s 20 Pages (Bandwidth may be reduced by controls) DC -  $2.5^{\circ}$  kHz for Sensor SC24/DC+AC 0.1 Hz -  $2.5^{\circ}$  kHz for Sensor SC11/AC 0.1 Hz - 2.5 KHz 0.1 Hz - 500 Hz 1.5 Hz - 2.5<sup>8</sup> kHz DC - 2.5<sup>8</sup> kHz XYZ/A upper/lower - all modes except narrow band Centre frequency, fo range: 1 Hz - 1250 Hz Accuracy:  $\pm 1\%$  within pass band, ( $f_0 \pm 3\%$ ) Attenuation: 60 dB min. in stop band, ( $f_0 \pm 20\%$ ) Waveform, RMS, Peak to Peak, Narrow band RMS, Narrow band Pk-Pk. Time, text string Clear chart data Indicates state of data acquisition buffer Page, scroll Pan, zoom, format, reset and clear chart Start: Now, At time, Triggered Stop: Period, File size, Disk space

Log rate limit, time step:  $\geq$  (page length)/500

 $\alpha$  g's are units of the acceleration due to gravity

 $^{\beta}$  <sup>4</sup> Channel mode only

 $\gamma$  Not available on 20000 Hz range in 8 channel mode

<sup>δ</sup> 1.25 kHz in 8 channel mode